

Avigo™ .014" Hydrophilic Guidewire Ordering Information

Reference Number	Diameter (in)	Total Length (cm)	Coil Length (cm)
103-0606-200	.014	205	5

Avigo™ .014" Hydrophilic Guidewire Device Details



GUIDEWIRE FUNDAMENTALS:

No kinks

Avoid wire kinking to promote peak performance.

Proper hydration

Hydrate for at least 30 seconds to provide adequate lubricity.

Tip Shape

Shape "with the ribbon" to maintain tip integrity.


The Hydrophilic Guidewire is indicated for general intravascular use to aid in the selective placement of catheters in the peripheral and cerebral vasculature during diagnostic and/or therapeutic procedures. The device is not intended for use in the coronary arteries.

Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device.

COVIDIEN, COVIDIEN with logo, Covidien logo and "positive results for life" are U.S. and internationally registered trademarks of Covidien AG. TM* Trademark of its respective owner. Other brands are trademarks of a Covidien company. © 2013 Covidien. 116713-001 (A) FEB/13



Avigo™ .014" Hydrophilic Guidewire

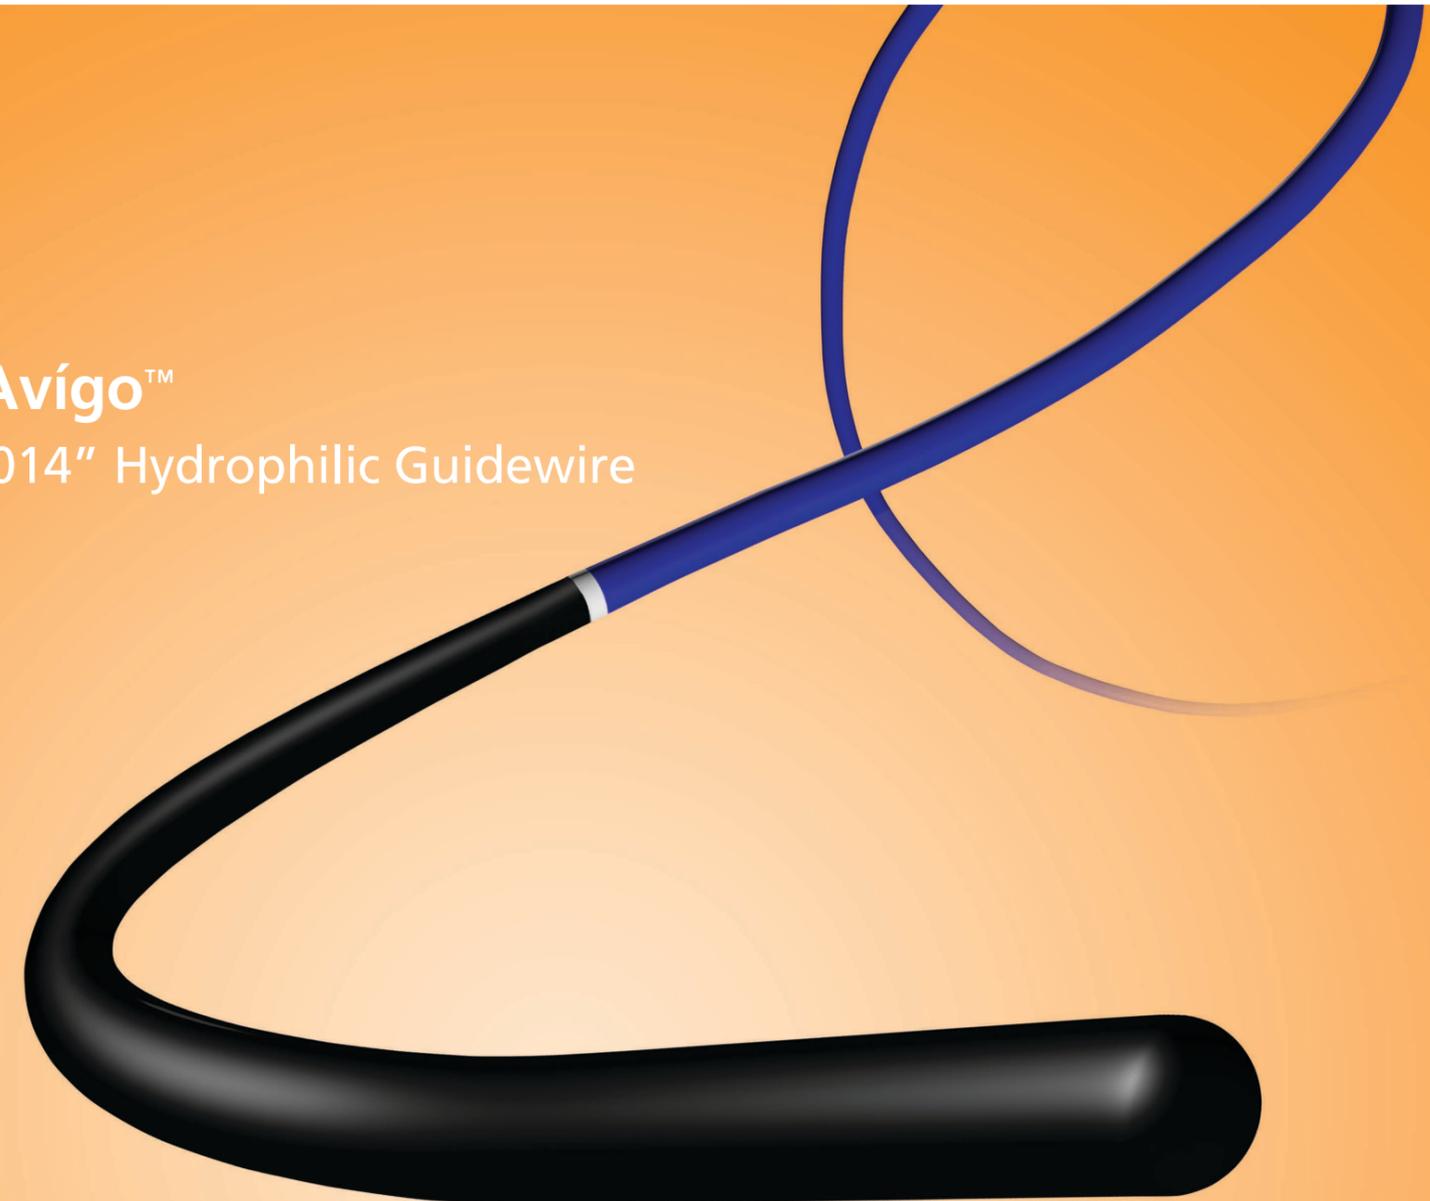

Every time you need support.





COVIDIEN
106/108 Rue la Boétie - 75008 PARIS
FRANCE

+33 1 56 88 51 30 [o]
+33 6 08 23 10 59 [m]

www.covidien.com

Offering a VERY SUPPORTIVE platform for delivering devices¹

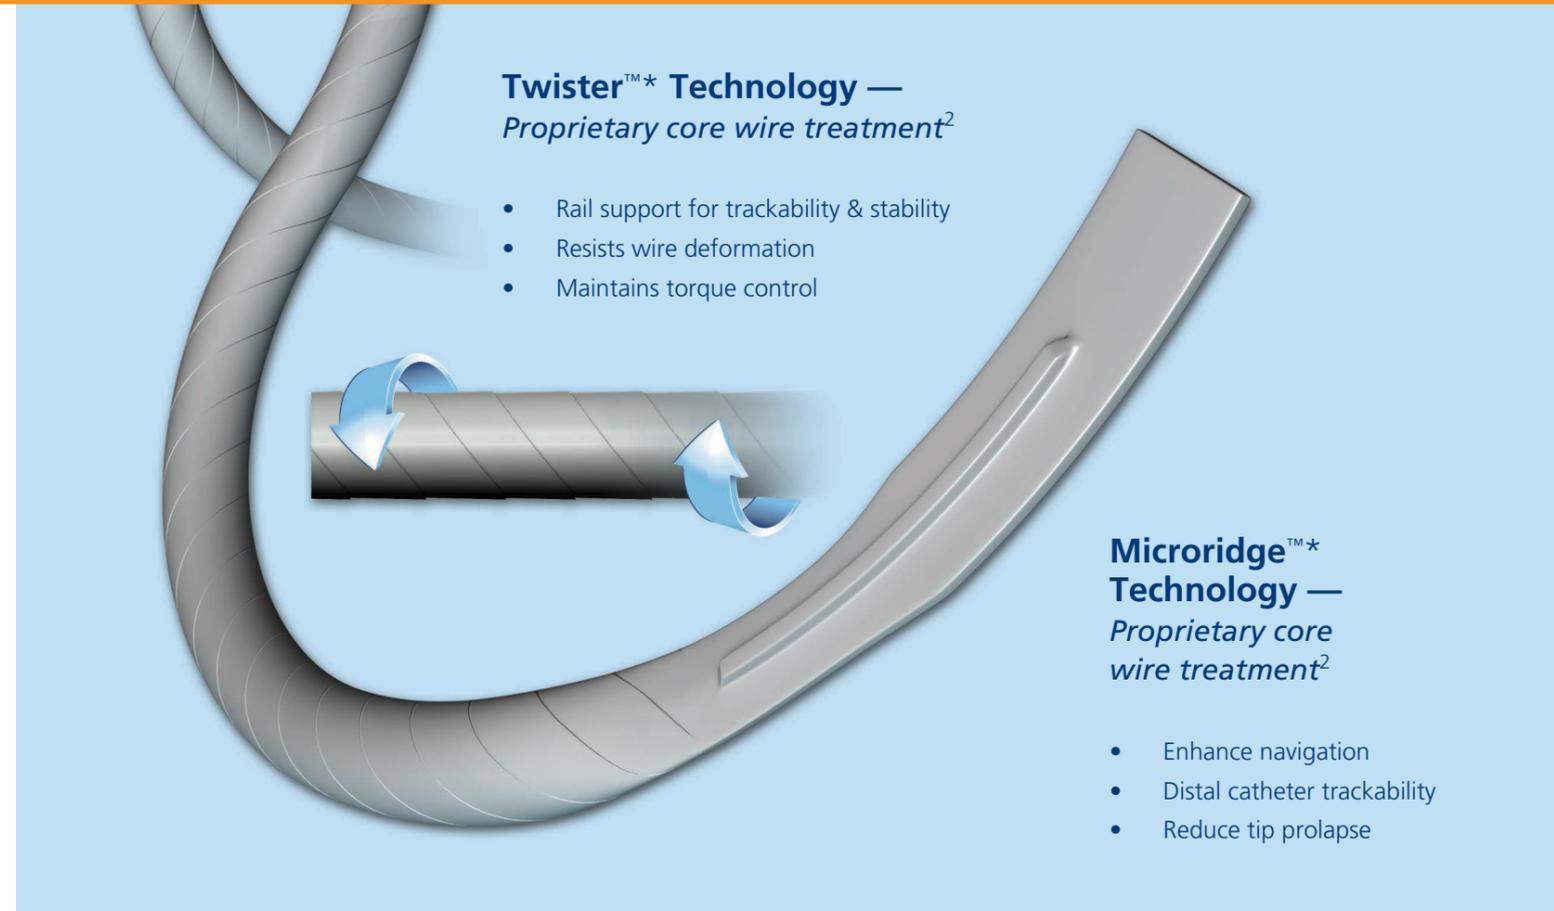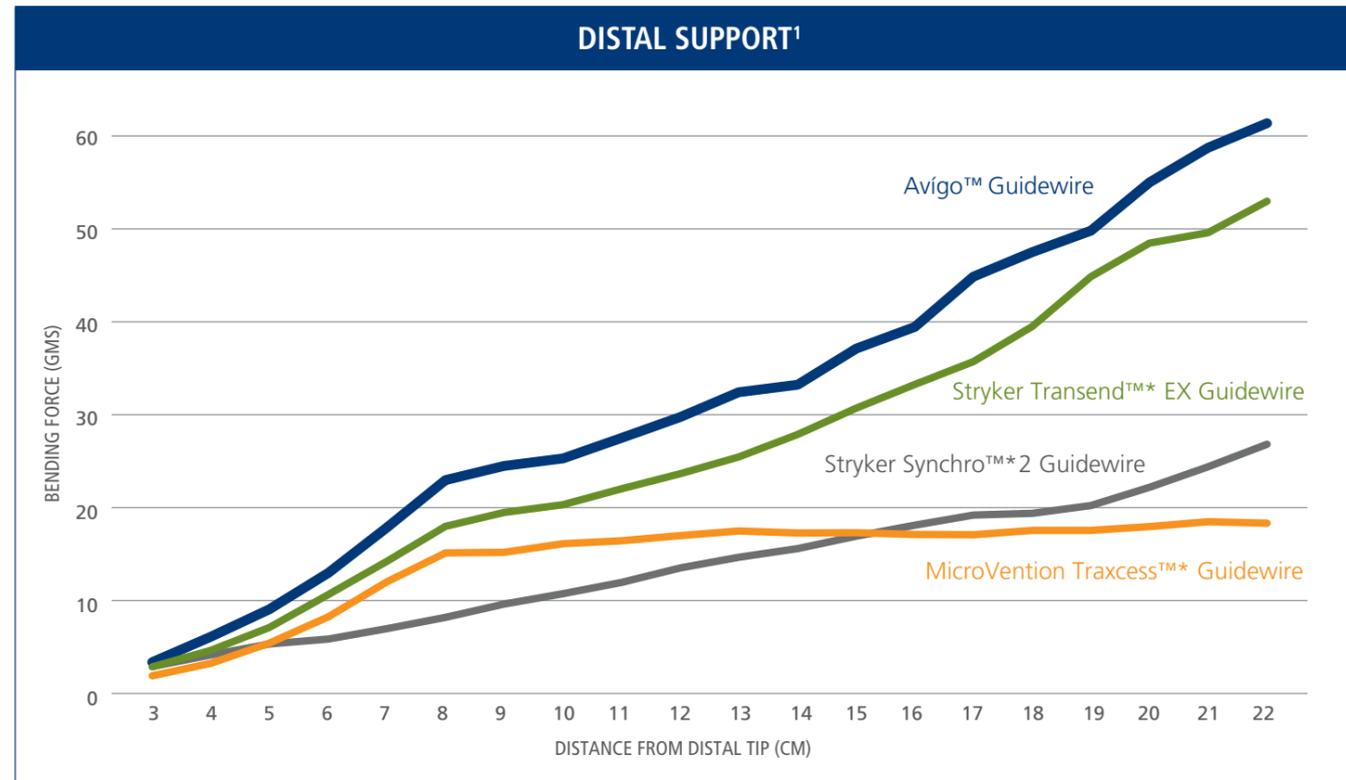

TRACKING
robust systems

The Avigo™ guidewire provides support for **tracking** 021 and 027 systems smoothly, for example with the Marksman™ catheter for Pipeline™ embolization device delivery or with the Orion™-21 micro catheter for stent delivery.

CROSSING
challenging clot

The Avigo™ guidewire provides support for **crossing** clot with reduced tip prolapse during catheter access for ischemic stroke cases.

MAINTAINING
catheter position

The Avigo™ guidewire's core wire design provides support for **maintaining** catheter stability during precise navigation, for example when selecting small or ruptured aneurysms or when navigating past wide-necked aneurysms.

38 cm Tungsten Doped Radiopaque Jacket²

- Soft radiopacity allows visualization of cerebral anatomy

5 cm Radiopaque Marker²

- Great tip visualization



¹ Based on internal comparative analysis; Tested vs. Transend™*, Traxcess™*, and Synchro™*. TRNV-10563, 3-Point Bend Test; Test results are averaged; n=10 per model. (2012) ² DWG50604